THERA TRAINER

CYCLING GROUP THERAPY SOFTWARE PACKAGE

USER MANUAL

EN English translation of original user manual

MADE IN GERMANY

Congratulations!

You've made a great choice by purchasing this software package. This innovative software package delivers maximum performance – Made in Germany.

This user manual should help you familiarize yourself with the software package. It takes you safely through the functions and use, and also offers plenty of tips and advice for getting the most out of your new software package.

Before using the Cycling Group Therapy software package, please read chapter 2 "Safety and Dangers."

If you have any further questions or comments, your trained specialized dealer will be happy to help.

We hope you will enjoy keeping active with your software package.

1 USER GUIDE 4
1.1 Warnings 4
1.2 Advice 4
1.3 Symbols in the user manual 4
1.4 Symbols on the product 5
2 SAFETY AND DANGERS 6
3 INTENDED USE 6
4 FORSEEABLE MISUSE 7
4.1 Misuse. 7
5 SCOPE OF DELIVERY AND EQUIPMENT 7
5.1 Scope of delivery 7
5.2 Basic equipment 7
6 STARTUP 7
6.1 Startup 7
6.2 Requirements. 8

USER PART. 9

7 OPERATION 10
7.1 Home screen 10
7.2 Starting therapy session 11
7.3 Shutting down the computer 13
8 BIOFEEDBACK ILLUSTRATIONS 14
8.1 Helicopter biofeedback illustration 14
8.2 Hill race biofeedback illustration 16
8.3 Bike tour biofeedback illustration 19

EXPERT PART 21

9 OPERATION 22
9.1 Logging in 22
9.2 Home screen 23
9.3 Setting up therapy sessions 24
9.4 Logging out 26

SERVICE PART 27

10 OPERATION 28
10.1 Logging in 28
10.2 Home screen 29
10.3 Adjusting the settings 30
10.4 Logging out 32
11 MAINTENANCE AND REPAIRS. 33
11.1 Maintenance 33
12 TROUBLESHOOTING 33
10.1 General errors 33
10.2 Software errors 33
13 TECHNICAL DATA 34
13.1 Installation requirements 34
14 STANDARDS AND LEGISLATION 34
15 DISPOSAL 34
16 WARRANTY 34

1 USER GUIDE

The user manual and product are marked with a variety of symbols. These symbols and their functions help you to use the product safely and efficiently.

1.1 Warnings

Warning categories

Warnings have different signal words depending on the type of danger:

- ❑ **Caution** warns of damage to property.
- ❑ **Warning** warns of physical injury.
- ❑ **Danger** warns of danger to life.

Structure of warnings

Signal Word

Type and Source of Danger!

▶ Measure for avoiding the danger.

1.2 Advice

Advice *Information for efficient use of the product.*

1.3 Symbols in the user manual

Instructions

Structure of instructions:

▶ Guidance for an activity.

Presentation of results if required.

Lists

Structure of non-numbered lists:

- ❑ List level 1
  - – List level 2

Structure of numbered lists:

1. List level 1
2. List level 1
   2.1 List level 2
   2.2 List level 2

USER PART

- ❑ Describes handling and use for users or therapy assistants.

EXPERT PART

- ❑ Describes handling and use for specialized staff e. g. doctors or therapists.

SERVICE PART

- ❑ Describes handling and use for the trained specialized dealer in the case of servicing, e. g. service employee.

1.4 Symbols on the product

	User manual
	Follow the user manual!
	Manufacturer
	Date of manufacture
	Market launch in accordance with Medical Devices Directive 93/42/EEC
	Disposal Do not dispose of the product in household waste. Dispose of the product in accordance with local regulations.

2 SAFETY AND DANGERS

- ▶ Follow the user manual.
- ▶ Use software in an undamaged and functional status only.
- ▶ Use software on the installed system only.
- ▶ Specialized staff should perform induction training before initial startup.
- ▶ Clarify training duration with doctor or therapist.
- ▶ Before starting training, ensure that an assistant or specialized staff are available to operate the device.
- ▶ The assistant should be trained by specialized staff before initial startup.
- ▶ In the case of damage, faults, etc. in the software, contact the specialized dealer immediately.
- ▶ If you experience symptoms of illness during or after training, consult a doctor immediately.
- ▶ End the session if the user becomes fatigued during training.
- ▶ Allow children to train under supervision only.
- ▶ Use only the manufacturer's original software.
- ▶ Do not combine the software with other software.
- ▶ Only use the software in conjunction with the THERA-Trainer tigo or THERA-Trainer veho.
- ▶ Adjust the biofeedback illustrations according to user fitness level.
- ▶ Follow the safety advice for operating the THERA-Trainer tigo or THERA-Trainer veho.

3 INTENDED USE

The software:

- ❑ is used to visualize user activity with the THERA-Trainer tigo or THERA-Trainer veho.
- ❑ is used, in conjunction with a computer and the wireless transfer of training data (such as number of revolutions, etc.) with the THERA-Trainer tigo or THERA-Trainer veho, to mobilize people whose mobility is limited after accidents, operations, or general illnesses affecting the musculoskeletal system.

Advice *Follow the indications of the THERA-Trainer tigo or THERA-Trainer veho.*

Users

- ❑ People who are authorized to use and train with the software with appropriate instruction from specialized staff.
- ❑ The user is fully responsible for the safe and intended use of the software.

Specialized Staff

- ❑ People who have acquired their knowledge through specialized training in the medical or medical technology sector (e.g. doctors, therapists, specialized dealers).
- ❑ People who can identify safety-relevant regulations and possible dangers at work (e. g. assistants) based on professional experience and instruction/training from the manufacturer.
- ❑ For safe use of the software, specialized staff must be trained in regular intervals.

4 FORSEEABLE MISUSE

The software should not be used for:

- ❑ Diagnosis
- ❑ Monitoring
- ❑ Measurement

4.1 Misuse

Do not use the software with products:

- ❑ which emit ionizing radiation (e.g. radiotherapy, nuclear medicine, etc.)
- ❑ in rooms with
  - explosive substances
  - enriched oxygen
- ❑ in the presence of
  - flammable anesthetics
  - volatile solvents

Do not use the software with a computer and display unit within the patient environment without a medical power supply.

5 SCOPE OF DELIVERY AND EQUIPMENT

Delivery includes the Cycling Group Therapy software package.
This user manual describes all functions and operating options of the software.

5.1 Scope of delivery

The delivery note contains all information about the scope of delivery.

5.2 Basic equipment

- ❑ Cycling Group Therapy software
- ❑ Licence file
- ❑ 4 x Bluetooth sticks
- ❑ USB-stick with software update THERA-Trainer tigo / THERA-Trainer veho
- ❑ Start number stickers for Cycling Group Therapy
- ❑ User manual for the Cycling Group Therapy software package

6 STARTUP

6.1 Startup

The Cycling Group Therapy software package is installed on a computer by the manufacturer.

▶ For a subsequent installation on a computer approved by the manufacturer, follow the installation instructions provided.

6.2 Requirements

Hardware

To install and use the software on a computer, the following system requirements must be met:

- ❑ Intel Pentium / 2.6 GHz (dual core) or similar
- ❑ Intel HD Graphics Dynamic Video Memory Technology 5.0 or similar
- ❑ 4 GB RAM
- ❑ 160 GB HDD space
- ❑ Bluetooth dongle supported by 32feet.NET
- ❑ Bluetooth 2.0
- ❑ Windows 7 Home or Windows 8

Advice *A video projector or screen is required for displaying the biofeedback illustrations.*

Use of the computer/display unit within the patient Environment (<1.5 m circumference around the device)

- ❑ Computer/display unit conforms to DIN EN 60601-1.

  -or-

- ❑ Standard computer/display unit in accordance with DIN EN 60950, which can only be used in conjunction with a suitable medical isolating transformer, with basic insulation in accordance with DIN EN 60601-1.
- ❑ No electrical devices are connected to the computer/display unit (e. g. printer or network connections).
  - – Other electrical devices are only permitted if they are galvanically isolated in accordance with DIN EN 60601-1

    -or-

  - – Devices are operated via an isolating transformer in accordance with DIN EN 60601-1.

Use of the computer/display unit outside the patient Environment (>1.5 m circumference outside the device)

- ❑ Computer/display unit conforms to DIN EN 60601-1.

  -or-

- ❑ Standard computer/display unit in accordance with DIN EN 60950.

Advice *Deviations from the requirements specified above are the sole responsibility of the operator.*

THERA-Trainer tigo or THERA-Trainer veho

The following requirements must be met in order to use the software with the THERA-Trainer tigo or THERA-Trainer veho:

- ❑ The software version of THERA-Trainer tigo or THERA-Trainer veho must be at least 3.1.x.
- ❑ Control and display unit with 10.4" color screen incl. touch function.

USER PART

The user part describes software handling for users or therapy assistants. **Advice**

7 OPERATION

7.1 Home screen

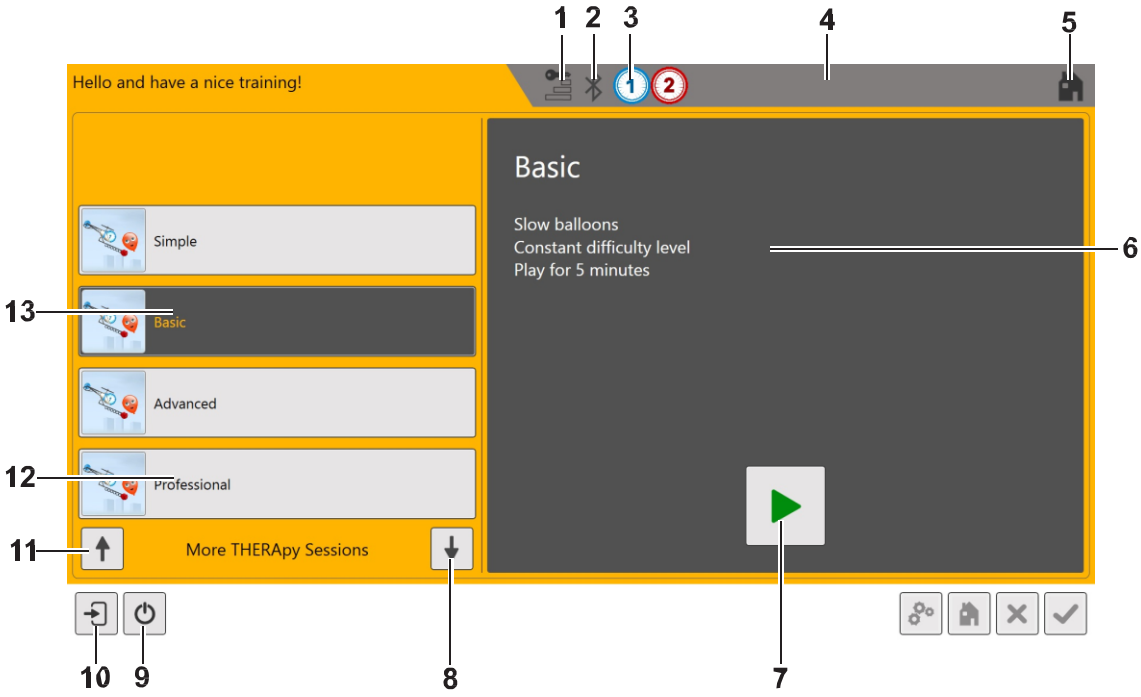

(1) Login status
(2) Bluetooth connection available
(3) Display of which start numbers of the THERA-Trainer tigo or THERA-Trainer veho are connected to the software
(4) Status line (current area, login status, etc.)
(5) Symbol of the current area (Home/Home screen)
(6) Description of the therapy session
(7) Start therapy session button
(8) Down button
(9) Shut down computer button
(10) Login button
(11) Up button
(12) Selectable therapy sessions
(13) Currently selected therapy session

Advice *Buttons with a grey background are inactive (inactive → , active →).*

7.2 Starting Therapy Sessions

To start therapy sessions, ensure that

- the user is secured in THERA-Trainer tigo or THERA-Trainer veho.
- an assistant is available.
- there is a connection between the THERA-Trainer tigo or THERA-Trainer veho and the software.
- the settings for the user's individual requirements have been made on the THERA-Trainer tigo or THERA-Trainer veho.

To start a therapy session with the helicopter biofeedback illustration or hill race biofeedback illustration:



- Select a therapy session.
- Click on button **1**.

The THERA-Trainer tigo or THERA-Trainer veho and the software are connected now.

- Follow the instructions below.

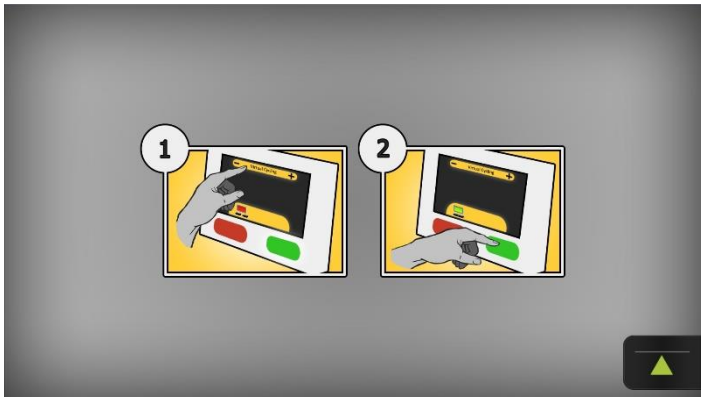

1. Select the "Group Therapy" training program on the THERA-Trainer tigo or THERA-Trainer veho. See the THERA-Trainer tigo or THERA-Trainer veho user manual.
2. Press the START button on the control and display unit.

All available THERA-Trainer tigo or THERA-Trainer veho are now shown on the left side (start number 1 – 4).

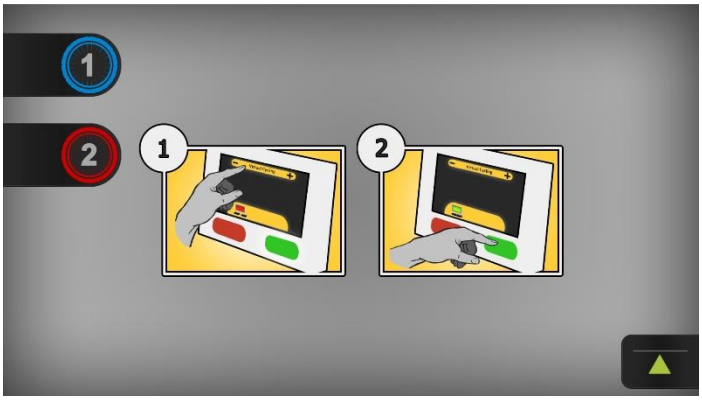

Advice

Up to four THERA-Trainer tigo or THERA-Trainer veho can be used for training with the software at the same time.

Removing/Adding THERA-Trainer tigo or THERA-Trainer veho:

- ▶ Click on button **1**.
- ▶ The THERA-Trainer tigo or THERA-Trainer veho with the corresponding start number is removed from training.
- ▶ Button **1** changes to button **2**.
- ▶ The THERA-Trainer tigo or THERA-Trainer veho with the corresponding start number is now inactive.
- ▶ If you click again on button **2** with the same start number, this THERA-Trainer tigo or THERA-Trainer veho will become active again.

The following screen is now displayed.

- ▶ If all the required THERA-Trainer tigo or THERA-Trainer veho have been removed/added, press button **3**.
- ▶ The therapy session starts.

To stop the therapy session:

- ▶ Move the mouse pointer over button **4**. A window opens on the right side (see right image).
- ▶ Press button **5** to leave the screen and stop the therapy session.

Advice

Before pressing START, it is essential to check that the user is sufficiently safe with the THERA-Trainer tigo or THERA-Trainer veho.

To start a therapy session with the "bike tour" biofeedback illustration:

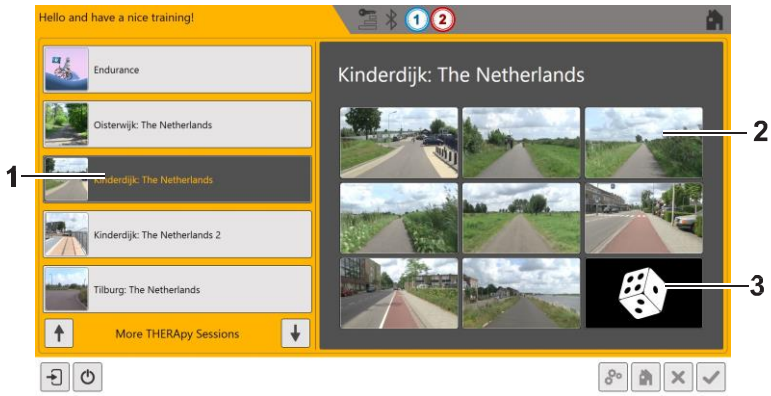

- ▶ Select a therapy session **1**.
- ▶ Select the landscape you want **2**.
- ▶ The therapy session starts.
- ▶ If you can't decide which landscape to use or if you are happy with a random choice, select dice **3**. The therapy session starts.

7.3 Shutting down the computer

To shut down the computer,

- ▶ Click on button **4**.

8 BIOFEEDBACK ILLUSTRATIONS

The following biofeedback illustrations can be selected as therapy sessions:

Helicopter biofeedback illustration

Hill race biofeedback illustration

Bike tour biofeedback illustration

8.1 Helicopter Biofeedback Illustration

Use the helicopter biofeedback illustration for:

- ❑ Short interval training.
- ❑ Improving coordination.
- ❑ Simultaneous training between 1 – 4 THERA-Trainer tigo or THERA-Trainer veho. Users can train with each other regardless of whether the setting is leg or upper body training.

Objective of the helicopter biofeedback illustration:

- ❑ Move the helicopter up or down by changing the number of revolutions in order to box the balloon away.

Advice *If the helicopter is no longer able to reach the balloon, it will fly into the thorns and burst.*

Helicopter biofeedback illustration:

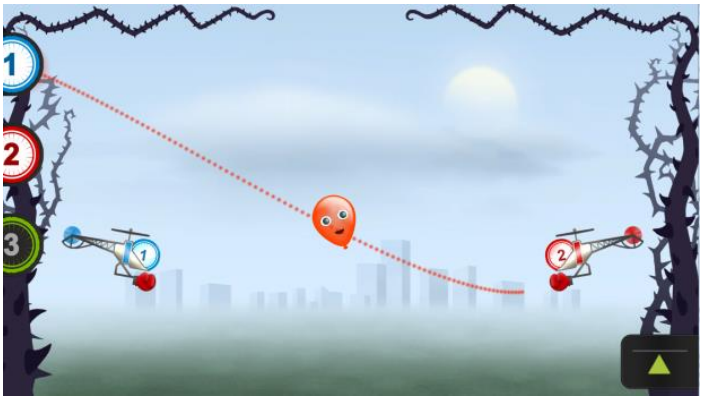

- ❑ All THERA-Trainer tigo or THERA-Trainer veho connected to the software are shown on the left side (here start numbers 1 – 3).
- ❑ Active THERA-Trainer tigo or THERA-Trainer veho are shown with a white background on the start number (here start numbers 1 and 2).
- ❑ THERA-Trainer tigo or THERA-Trainer veho which are not active are shown with a grey background on the start number (here start number 3).

Control the helicopter as follows:

- ▶ Move the helicopter upward by active pedaling (increasing the number of revolutions).
- ▶ Move the helicopter downward by reducing the number of revolutions (slower pedaling but not braking).
- ▶ Reduce resistance on the THERA-Trainer tigo or THERA-Trainer veho if the helicopter cannot be moved all the way up. The highest speed can also be set on the software (see Setting highest speed).

Advice

Switch off spasm detection on the THERA-Trainer tigo or THERA-Trainer veho. The THERA-Trainer tigo or THERA-Trainer veho now reacts at a very late stage to a crank handle block.

Adding/Removing users during training:

- ▶ Click button **1** (start number with a grey background) to add another user. The THERA-Trainer tigo or THERA-Trainer veho is now added to training as a helicopter with the corresponding start number.
- ▶ Click button **2** (start number with a white background) to remove a user from training. The THERA-Trainer tigo or THERA-Trainer veho is now removed from training as a helicopter with corresponding start number.

Setting highest speed:

- ▶ Move the mouse pointer over button **3**.
- ▶ Button **3** opens. Click the arrows on button **3** to set the user's highest speed (rpm).
- ▶ The helicopter is right at the top of the screen when the highest speed is reached.

Advice

Setting the highest speed has no impact on the number of revolutions on the THERA-Trainer tigo or THERA-Trainer veho.

Level of Difficulty:

- ❑ The more balloons protected from the thorns, the greater the level of difficulty.
- ❑ The balloons get faster when a new level of difficulty is reached.
- ❑ As soon as the helicopter can no longer reach the balloons, they slow down again.

Stopping/Ending a therapy session:

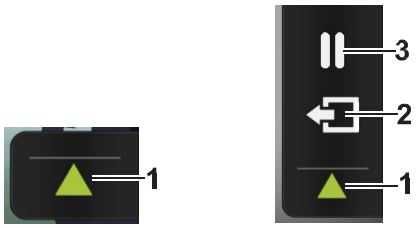

- ▶ Move the mouse pointer over button **1**. A window opens on the right side (see right image).
- ▶ Click on button **3** to stop the therapy session (pause).
  Click on button **3** again to continue the therapy session.
- ▶ End training with button **2**.

When training has ended, the following training evaluation is displayed:

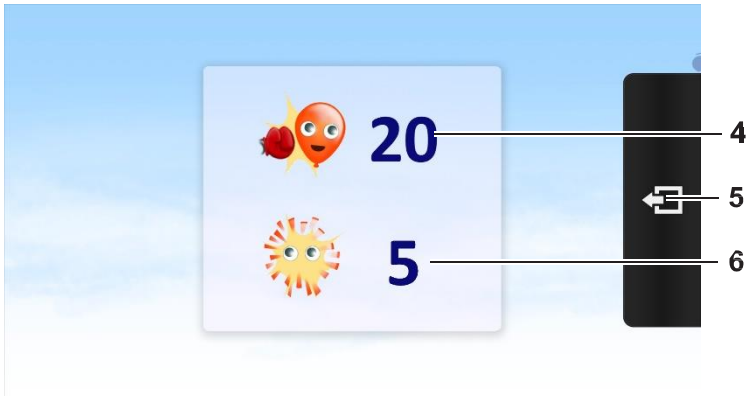

- ❑ Display **4** shows how many balloons were successfully boxed away.
- ❑ Display **6** shows how many balloons burst.
- ❑ Exit this screen with button **5**.

8.2 Hill race biofeedback illustration

Use the hill race biofeedback illustration for:

- ❑ Longer active training.
- ❑ Improving coordination. Overly fast and uncoordinated pedaling is displayed.
- ❑ Simultaneous training between 1 – 4 THERA-Trainer tigo or THERA-Trainer veho. Users can train with each other regardless of whether the setting is leg or upper body training.

Objective of the hill race biofeedback illustration:

- ❑ Cycle to the destination as quickly as possible by means of targeted, active, and coordinated pedaling with the THERA-Trainer tigo or THERA-Trainer veho. The first bike to reach the destination gets a gold medal.

Hill race biofeedback illustration:

- ❑ All THERA-Trainer tigo or THERA-Trainer veho connected to the software are shown on the left side (here start numbers 1 – 4).
- ❑ Active THERA-Trainer tigo or THERA-Trainer veho are shown with a white background (here start numbers 1 and 4).
- ❑ Inactive THERA-Trainer tigo or THERA-Trainer veho are shown with a grey background on the start number.

Rest phases during the therapy session:

There is a rest phase between rounds depending on the therapy session. The following screen is displayed:

- ❑ Display **1**, current intermediate status of the rounds. (Example: 1st race → 2nd place; 2nd race → 1st place)
- ❑ Display **2**, remaining rest time.

Control the bike as follows:

- ▶ Move the bike forward by active pedaling (increasing the number of revolutions).

Too fast and uncoordinated training is displayed. The front wheel lifts up and the bike slows down. **Advice**

Adding/Removing users during training:

- ▶ Click button **1** (start number with a grey background) to add another user. The THERA-Trainer tigo or THERA-Trainer veho is now added to training as a bike with the corresponding start number.
- ▶ Click button **2** (start number with a white background) to remove a user from training. The THERA-Trainer tigo or THERA-Trainer veho is now removed from training as a bike with the corresponding start number.

Setting highest speed:

- ▶ Move the mouse pointer over button **3**.
- ▶ Button **3** opens. Click the arrows of button **3** to set the user's highest speed (rpm).
- ▶ If the highest speed is exceeded, the front wheel lifts up and the bike slows down.

Advice

Setting the highest speed has no impact on the number of revolutions on the THERA-Trainer tigo or THERA-Trainer veho.

Stopping/Ending a therapy session:



- ▶ Move the mouse pointer over button **4**. A window opens on the right side (see right image).
- ▶ Click button **6** to stop the therapy session (pause).
  Click on button **6** again to continue the therapy session.
- ▶ Exit training with button **5**.

When training has ended, the following training evaluation is displayed:

- ❑ Display **7** shows how many races have been won. (Example: 1st and 3rd races→ 1st place; 2nd race → 2nd place)
- ❑ Exit this screen with button **8**.

8.3 Bike tour biofeedback illustration

Use the bike tour biofeedback illustration for:

- ❑ Longer active training.
- ❑ Simultaneous training between 1 – 4 THERA-Trainer tigo or THERA-Trainer veho. Users can train with each other regardless of whether the setting is leg or upper body training.

Objective of the bike tour biofeedback illustration:

- ❑ Run the video faster or slower by changing the number of revolutions. The average speed of all participants is used for this.

The video runs at normal speed with an average speed of 40 rpm. **Advice**

Displaying/Hiding training time:

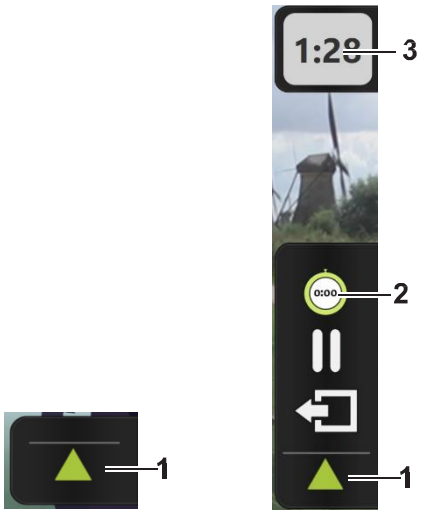

- ▶ Move the mouse pointer over button **1**. A window opens on the right side (see right image).
- ▶ Click on button **2** to display/hide the training time **3**.

Stopping/Ending a therapy session:

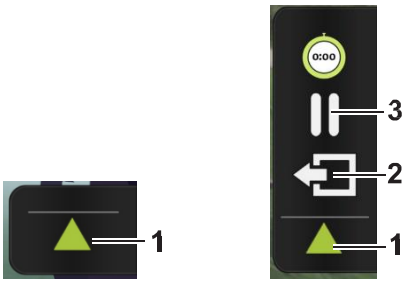

- ▶ Move the mouse pointer over button **1**. A window opens on the right side (see right image).
- ▶ Click on button **3** to stop the therapy session (pause).
  Click on button **3** again to continue the therapy session.
- ▶ End training with button **2**.

EXPERT PART

The expert part describes software handling for the doctor or therapist. **Advice**

9 OPERATION

9.1 Logging in

To access the login screen:

▶ Click on button **1**.

The password screen appears.

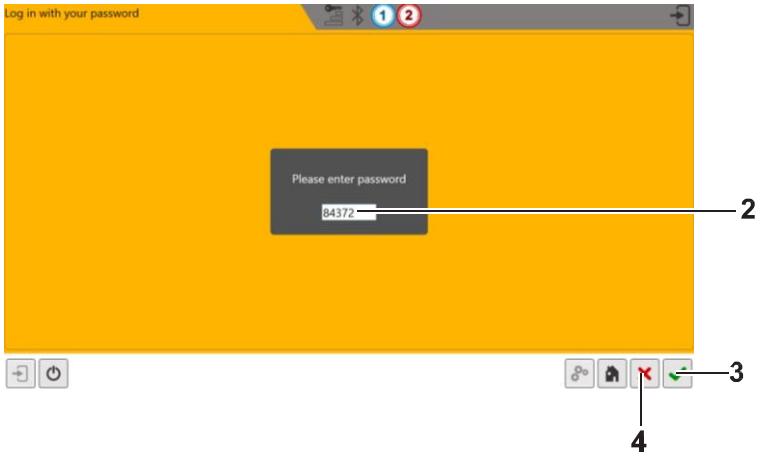

▶ Enter your password in field **2** (Password: **84372**).

▶ Confirm with button **3**.

▶ Cancel and return to the home screen with button **4**.

9.2 Home screen

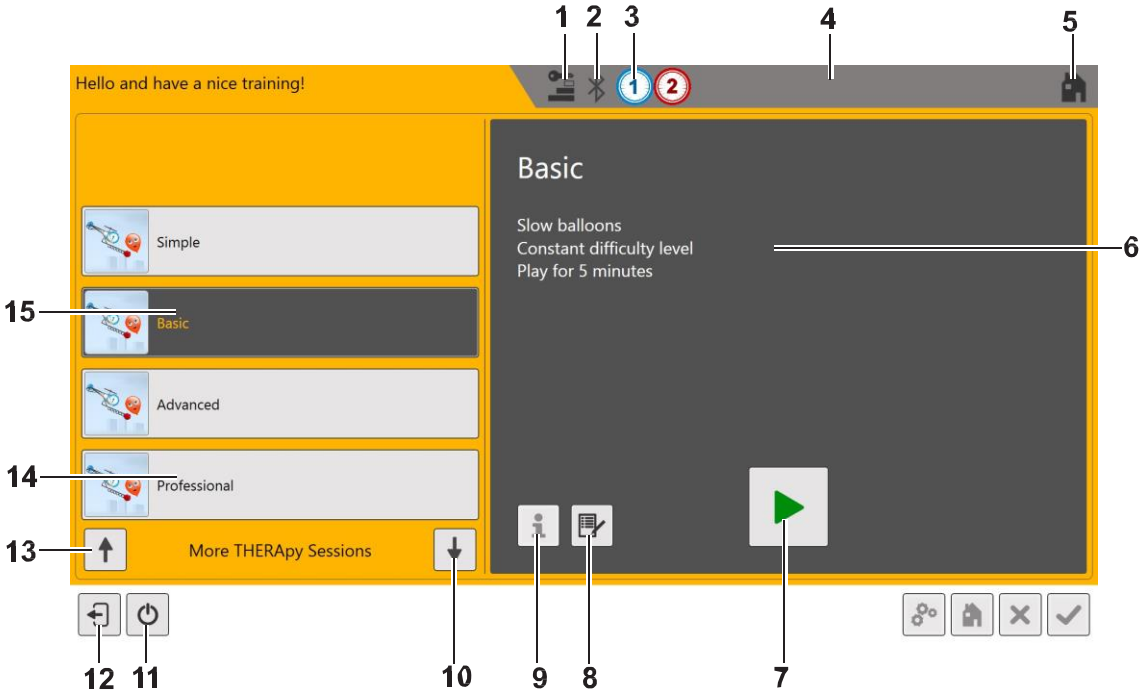

(1) Login status
(2) Bluetooth connection available display
(3) Display of which THERA-Trainer tigo or THERA-Trainer veho are connected to the software
(4) Status line (current area, login status, etc.)
(5) Symbol of the current area (Home)
(6) Description of the therapy session
(7) Start therapy session button
(8) Therapy session settings button (alternating with 9 active)
(9) Therapy session information button (alternating with 8 active)
(10) Down button
(11) Shut down computer button
(12) Log out button
(13) Up button
(14) Selectable therapy sessions
(15) Currently selected therapy session

Advice

Buttons with a grey background are inactive (inactive → , active →).

Logging in as specialized staff now also activates functions 8 and 9.

9.3 Setting up therapy sessions

Helicopter biofeedback illustration

To adjust settings for a therapy session with the helicopter biofeedback illustration:

- ▶ Select the therapy session.
- ▶ Click on button **1**.

The screen "Therapy session settings" appears.

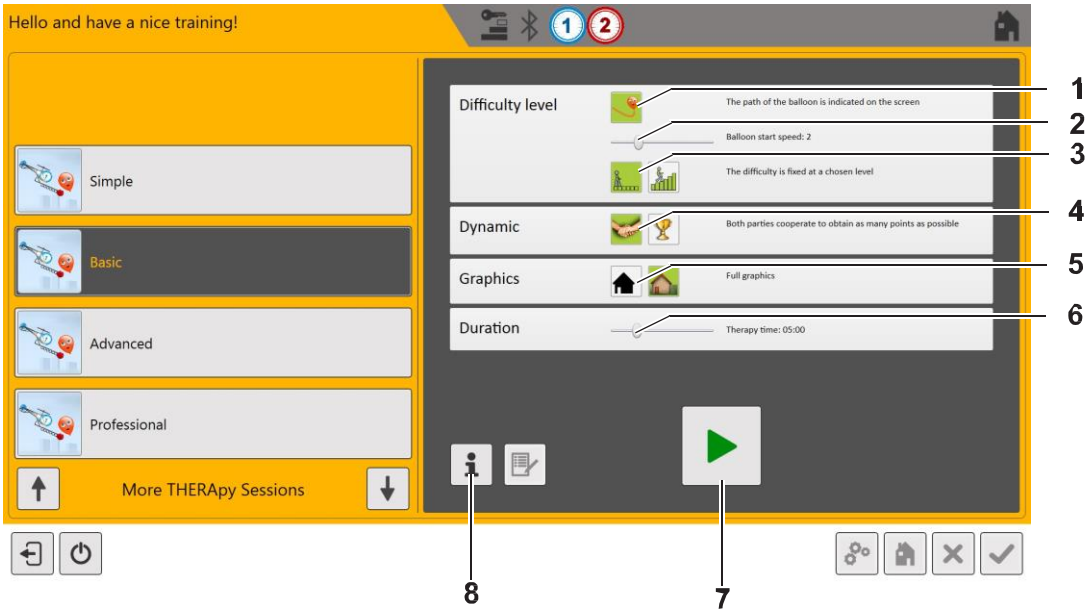

Adjust the settings as follows:

- ▶ Showing the path of the balloon on the screen can be switched on or off using button **1**.
- ▶ Set the start speed of the balloon with the slider **2**.
- ▶ Use button **3** to specify whether the level of difficulty should be adapted to user performance.
- ▶ Use button **4** to specify whether the users should train with or against one another.
- ▶ Use button **5** to specify whether simple or full graphics should be displayed.
- ▶ Set the training time with slider **6**.
- ▶ Display information about the therapy session with button **8**.
- ▶ Start the therapy session with button **7**.

Advice

The changed settings are not permanent. The default settings are active again after a change of therapy session.

Hill race biofeedback illustration

To adjust settings for a therapy session with the hill race biofeedback illustration:

- ▶ Select the therapy session.
- ▶ Click on button **1**.

The screen "Therapy session settings" appears.

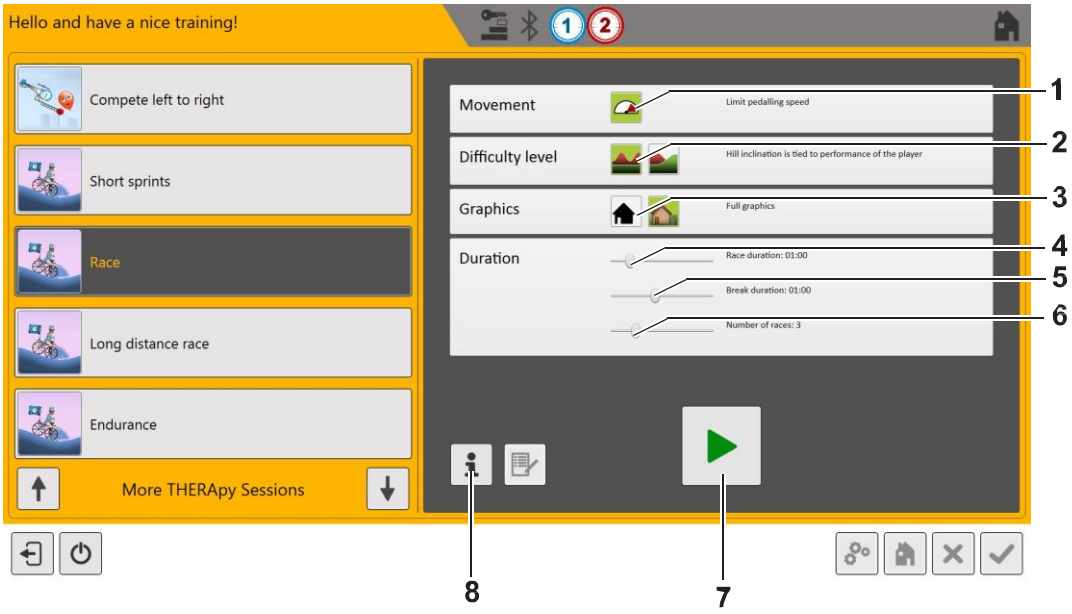

Adjust the settings as follows:

- ▶ Switch the highest speed limit on or off using button **1**.
- ▶ Use button **2** to specify whether the gradient of the hills should be adapted to user performance.
- ▶ Use button **3** to specify whether simple or full graphics should be displayed.
- ▶ Set the duration of the race with slider **4**.
- ▶ Set the rest phase (pause) with slider **5**.
- ▶ Set the number of races with slider **6**.
- ▶ Display information about the therapy session with button **8**.
- ▶ Start the therapy session with button **7**.

Advice

The changed settings are not permanent. The default settings are active again after a change of therapy session.

Bike tour biofeedback illustration

Advice

It is not possible to adjust settings for therapy sessions with the bike tour biofeedback illustration.

9.4 Logging out



Following completion:

▶ Click on button **1** to log out.

Software switches from expert part to user part.

SERVICE PART

Advice

The service part describes software handling for the trained specialized dealer in the case of servicing.

10 OPERATION

10.1 Logging in

To access the login screen:

▶ Click on button **1**.

The password screen appears.

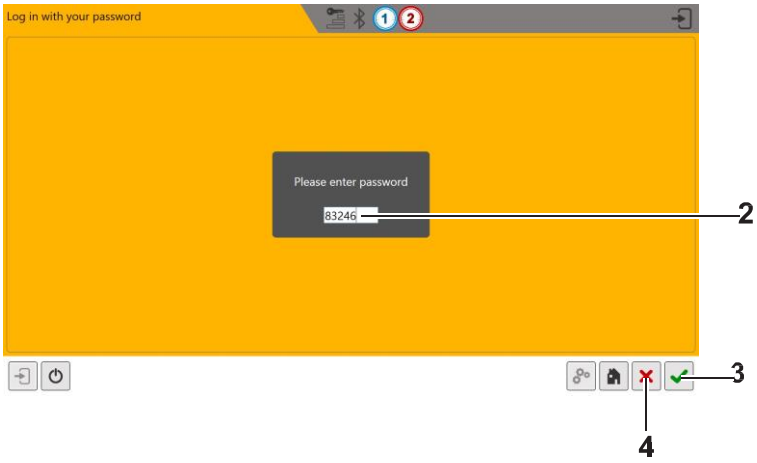

▶ Enter your password in field **2** (Password: **83246**).

▶ Confirm with button **3**.

▶ Cancel and return to the home screen with button **4**.

10.2 Home screen

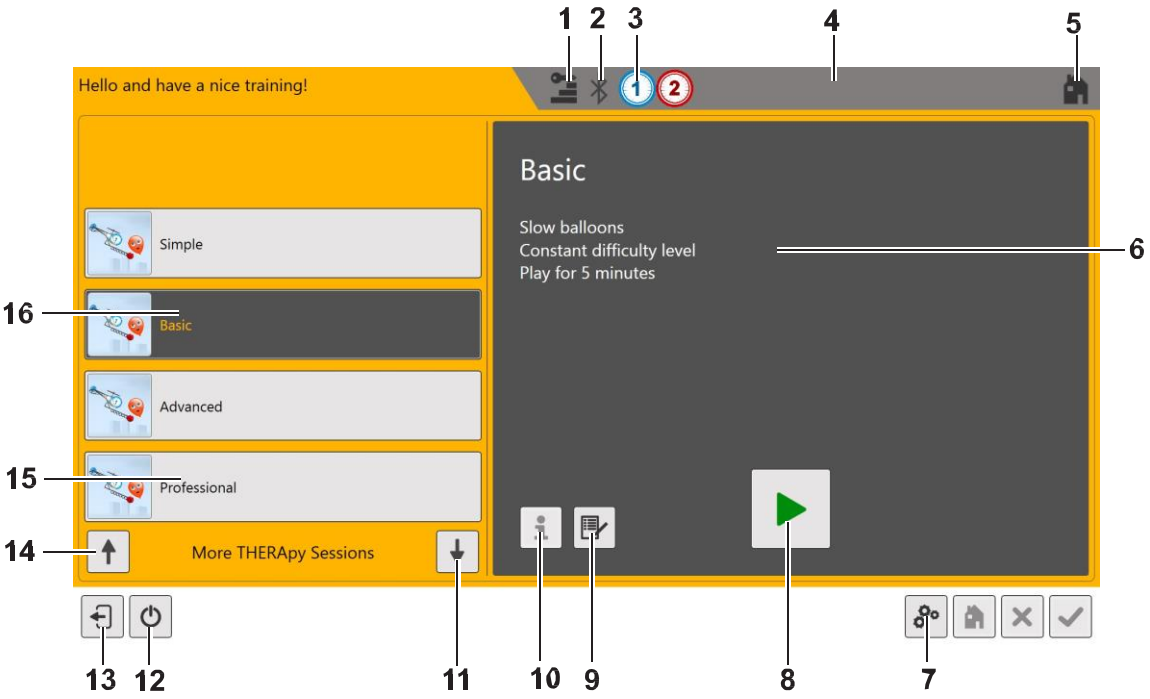

(1) Login status
(2) Bluetooth connection available display
(3) Display of which THERA-Trainer tigo or THERA-Trainer veho are connected to the software
(4) Status line (current area, login status, etc.)
(5) Symbol of the current area (Home/Home screen)
(6) Description of the therapy session
(7) Settings button
(8) Start therapy session button
(9) Therapy session settings button (alternating with 10 active)
(10) Therapy session information button (alternating with 9 active)
(11) Down button
(12) Shut down computer button
(13) Log out button
(14) Up button
(15) Selectable therapy sessions
(16) Currently selected therapy session

Advice

Buttons with a grey background are inactive (inactive → , active →).

Function 7 is also active when you log in as service staff.

10.3 Adjusting the Settings



To adjust the settings:

▶ Click on button **1**.

The "Select language" screen appears.

Selecting a language

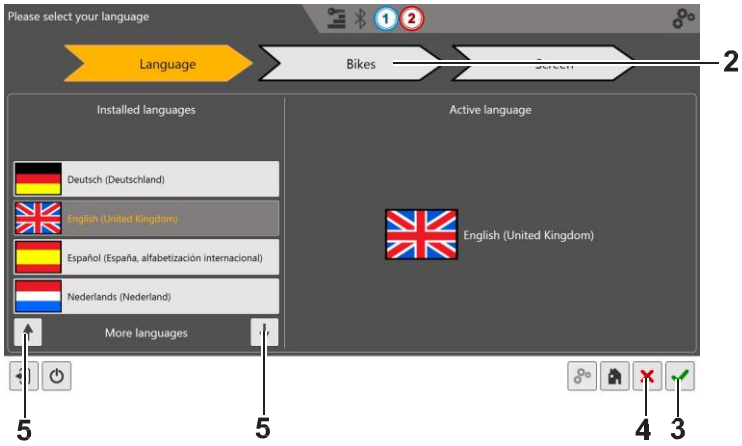

Select the language as follows:

▶ Select a preinstalled language. Additional languages can be displayed via button **5**.

▶ Adjust other settings with button **2**.

▶ Confirm the settings with button **3** and exit the screen.

▶ Cancel the settings and exit the screen with button **4**.

Selecting THERA-Trainer tigo or THERA-Trainer veho



To open the screen "Select bikes (THERA-Trainer tigo or THERA-Trainer veho)":

▶ Click on button **1**.

The screen "Select bikes (THERA-Trainer tigo or THERA-Trainer veho)" appears.

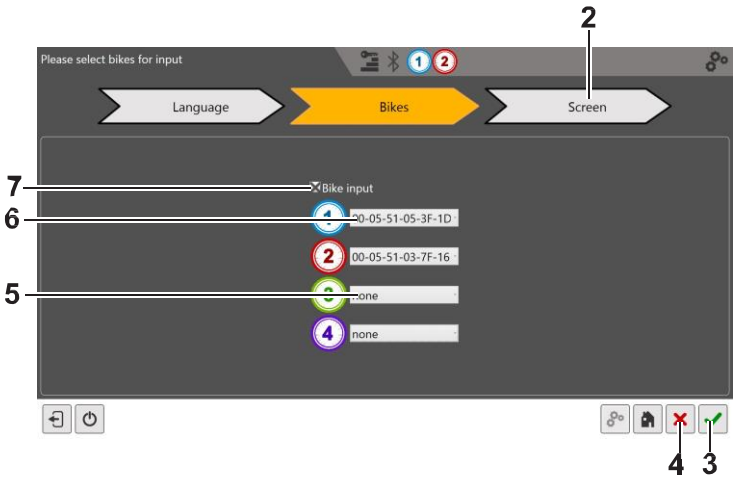

Select bikes (THERA-Trainer tigo or THERA-Trainer veho) as follows:

▶ Click on button **7** if the selection of bikes should be updated (e. g. if new THERA-Trainer tigo or THERA-Trainer veho should be added to the software). If button **7** is not selected, the selection of the bikes is not updated.

▶ Click on button **5** (for THERA-Trainer tigo or THERA-Trainer veho with start number 3).

▶ A list with an address for the THERA-Trainer tigo or THERA-Trainer veho is opened.

▶ Select the address. If several addresses are in the list, select the address which is not yet assigned.

▶ If an address is selected, this is shown in **6**.

▶ The software now detects that the THERA-Trainer tigo or THERA-Trainer veho is available with start number 3.

▶ Repeat this process with the other THERA-Trainer tigo or THERA-Trainer veho.

▶ Adjust other settings with button **2**.

▶ Confirm the settings with button **3** and exit the screen.

▶ Cancel the settings and exit the screen with button **4**.

Advice

Before the THERA-Trainer tigo or THERA-Trainer veho can be selected or connected to the software, the installation instructions must be followed.

As long as the THERA-Trainer tigo or THERA-Trainer veho or the control and display unit are not replaced, the addresses remain available for the software.

If the following message is displayed, proceed as follows:

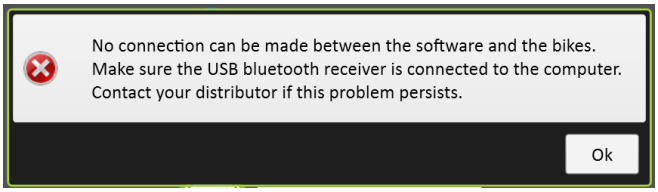
No connection can be made between the software and the bikes.
Make sure the USB bluetooth receiver is connected to the computer.
Contact your distributor if this problem persists.
Ok

- ▶ Check whether the computer is Bluetooth-enabled or whether a Bluetooth stick is inserted.
- ▶ If the computer is not Bluetooth-enabled, a Bluetooth stick must be inserted.
- ▶ If this message is still displayed, contact your trained specialized dealer.

Setting up the screen



To open the screen "Setting up the screen":

- ▶ Click on button **1**.

The screen "Setting up the screen" appears.

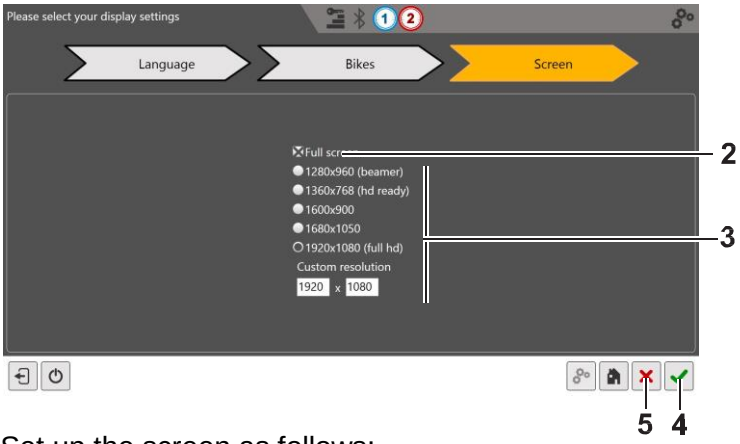

Set up the screen as follows:

- ▶ Click on button **2** to show the full-screen display.
- ▶ Use button **3** to select the screen resolution.
- ▶ Confirm the settings with button **4**.
- ▶ Cancel the settings and exit the screen with button **5**.

Advice *These settings only have to be changed if the display unit screen is replaced.*

10.4 Logging out



Following completion:

- ▶ Click on button **1** to log out.

Software switches from service part back to user part.

11 MAINTENANCE AND REPAIRS

11.1 Maintenance

The software does not require maintenance.

12 TROUBLESHOOTING

12.1 General errors

Error Code	Troubleshooting
Spasticity is displayed on the THERA-Trainer tigo or THERA-Trainer veho.	Spasticity is displayed on the THERA-Trainer tigo or THERA-Trainer veho. ❑ The current therapy session of the software is not terminated.
Voice-controlled emergency stop is displayed on the THERA-Trainer tigo or THERA-Trainer veho.	The voice-controlled emergency stop is displayed on the THERA-Trainer tigo or THERA-Trainer veho. ❑ The current therapy session of the software is not terminated.
Pause is displayed on the THERA-Trainer tigo or THERA-Trainer veho.	The STOP button on the THERA-Trainer tigo or THERA-Trainer veho was pressed once. ❑ The current therapy session of the software is not terminated.
Power cable is disconnected from the THERA-Trainer tigo or THERA-Trainer veho.	Power cable is disconnected from the THERA-Trainer tigo or THERA-Trainer veho during therapy session. ❑ The current therapy session of the software is not terminated.
Training is ended on the THERA-Trainer tigo or THERA-Trainer veho.	Training is ended by pressing the STOP button twice on the THERA-Trainer tigo or THERA-Trainer veho or if the training time has elapsed. ❑ The current therapy session of the software is terminated/ended.

12.2 Software errors

Error Code	Troubleshooting
Error	An error has occurred. Please restart. ❑ Contact your trained specialized dealer if this message does not disappear.
Error_Bluetooth	No connection between software and THERA-Trainer tigo or THERA-Trainer veho. ❑ Check whether a Bluetooth stick is inserted in the control and display unit with 10.4" color screen incl. touch function. ❑ Check whether the computer is Bluetooth-enabled. If not, a Bluetooth stick must be inserted. ❑ Contact your trained specialized dealer if this message does not disappear.
Not licensed!	The software is not licensed. ❑ Contact your trained specialized dealer.

13 TECHNICAL DATA

13.1 Installation requirements

	Cycling group therapy software package
Processor:	Intel Pentium / 2.6 GHz (dual core) or similar
Working memory:	4 GB RAM
Fixed-disk storage:	160 GB HDD space
Connections:	Bluetooth dongle supported by 32feet.NET Bluetooth 2.0
Operating system:	Windows 7 or Windows 8
Software version:	Software 1.0.x
THERA-Trainer tigo or THERA-Trainer veho software version	3.1.x

14 STANDARDS AND LEGISLATION

The software meets the following standards:

- ❑ Directive 93/42/EEC
- ❑ DIN EN 62304
- ❑ DIN EN ISO 13485

15 DISPOSAL

To dispose of the data medium:

- ▶ Comply with country-specific rules and regulations.
- ▶ Dispose of metal parts as scrap metal.
- ▶ Dispose of plastic parts according to the material.
- ▶ Dispose of electrical and electronic components as electronic waste.

16 WARRANTY

The manufacturer offers a manufacturer's guarantee that corresponds to statutory provisions. This is based on the delivery date.

During this time the manufacturer will replace faulty software free of charge.

The following are excluded from the manufacturer's guarantee:

- ❑ Opened devices
- ❑ Third-party installations and attachments
- ❑ Devices not repaired by trained specialized dealers.
- ❑ Damage caused by improper use.

NOTICES

MANUFACTURER:

THERA-Trainer®

a trademark of
medica Medizintechnik GmbH

Blumenweg 8
88454 Hochdorf
Germany

Phone: +49 7355-93 14-0
Fax: +49 7355-93 14-15

E-mail: info@thera-trainer.de
Internet: www.thera-trainer.de

Software: 1.0.x
Version: 01/2014

For declarations of conformity, see www.thera-trainer.de